

LLC-PK1 Kidney Cytotoxicity Assay

AUTHORED BY:	DATE:
Vu To, Geir Klinkenberg	13-05-2016

REVIEWED BY:	DATE:
Matthias Roesslein	14-05-2016
Rainer Ossig	
Sabrina Gioria	

APPROVED BY:	DATE:
Matthias Roesslein	14-05-2016

DOCUMENT HISTORY

Effective Date	Date Revision Required	Supersedes
DD/MM/YYYY	DD/MM/YYYY	DD/MM/YYYY

Version	Approval Date	Description of the Change	Author / Changed by
1.0	13.05.2016	All Initial Document	Geir Klinkenberg

Document Type	Document ID	Version	Status	Page
SOP	EUNCL-GTA-001	1.0		1/15

Table of Content

1	Introduction.....	3
2	Principle of the Method.....	3
3	Applicability and Limitations (Scope)	3
4	Related Documents	3
5	Equipment and Reagents.....	4
5.1	Equipment and Culture ware.....	4
5.2	Reagents	4
5.3	Reagent Preparation.....	4
6	Procedure	6
6.1	Flow chart	6
6.2	Cell handling	6
6.3	Cell seeding.....	7
6.4	Assay procedure	8
6.5	Calculations	10
7	Quality Control, Quality Assurance, Acceptance Criteria	10
8	Health and Safety Warnings, Cautions and Waste Treatment	11
9	Abbreviations	11
10	References.....	12
11	Appendix	13
11.1	Cell handling and storage	13
11.1.1	Cell origin and provenance.....	13
11.1.2	Thawing Procedure.....	13
11.1.3	Propagation of stock ampoules.....	14
11.1.4	Plate map with positioning of samples and controls in assay plates	15

Document Type	Document ID	Version	Status	Page
SOP	EUNCL-GTA-001	1.0		2/15

1 Introduction

This protocol describes the cytotoxicity testing of nanoparticle formulations in porcine proximal tubule cells (LLC-PK1), as part of the in vitro EU-NCL preclinical characterization cascade. The protocol utilizes two methods for estimation of cytotoxicity, 3-(4,5-Dimethyl-2-thiazolyl)-2,5-diphenyl-2H-tetrazolium bromide (MTT) reduction and lactate dehydrogenase (LDH) release [1-2].

2 Principle of the Method

1. MTT Assay

MTT is a yellow, water-soluble tetrazolium dye that is reduced by live cells to a water-insoluble, purple formazan. The amount of formazan can be determined by solubilizing it in DMSO and measuring it spectrophotometrically. Comparisons between the spectra of treated and untreated cells can give a relative estimation of cytotoxicity [3].

2. LDH Assay

LDH is a cytoplasmic enzyme that is released into the cytoplasm upon cell lysis. The LDH assay, therefore, is a measure of membrane integrity. The basis of the LDH assay: a) LDH oxidizes lactate to pyruvate, b) pyruvate reacts with the tetrazolium salt INT to form formazan, and c) the water-soluble formazan dye is detected spectrophotometrically [4, 5].

3 Applicability and Limitations (Scope)

The SOP describes in vitro methods for evaluation of cytotoxicity of nanoparticle formulations using the MTT (metabolic activity) and LDH-assays (membrane activity) for LLC-PK1 cells. For both assays, potential interferences of the nano formulations on the assay readout should be taken into account during design of experiments and interpretation of data. Existing available literature should therefore be reviewed during design of experiments in order to evaluate the applicability of the assays. The assays provide basic information of the cytotoxicity of the nanoparticle formulations. The assays does not provide information of sub lethal cellular effects or detailed mechanistic information of the toxic effect experienced by the cells.

4 Related Documents

Table 1:

Document Type	Document ID	Version	Status	Page
SOP	EUNCL-GTA-001	1.0		3/15

Document ID	Document Title
EUNCL-GTA-2	<i>Hep G2 Hepatocarcinoma Cytotoxicity Assay</i>

5 Equipment and Reagents

5.1 Equipment and Culture ware

1. Costar 96 well flat bottom cell culture plates (Nunc, 3598)
2. Greiner 96 well flat bottom polystyrene plates (Greiner, 655163)
3. Half area 96 well plate (Costar, 3695)
4. Plate reader (Tecan Infinity 200 Pro - or equivalent)
5. Orbital plate shaker
6. Incubator, 37°C with 5% CO₂ and 95% humidity

5.2 Reagents

1. LLC-PK1 (pig kidney cells) (LGC Standards, CL-101, LOT 59681631)
2. MTT (3-(4,5-dimethyl-2-thiazolyl)-2,5-diphenyl-2H-tetrazolium bromide) (Sigma, M5655)
3. Dimethyl sulfoxide (Sigma, D5879)
4. Glycine (Sigma, G7126 or G7403)
5. Sodium chloride (Sigma, S7653)
6. 10% Triton-X-100 (Sigma, 93443)
7. Digitonin (Sigma, D141-500MG)
8. Medium 199 Cell culture media (Sigma, M2154)
9. Fetal bovine serum (Sigma, F7524, LOT 025M3302)
10. L-Glutamine (Sigma, G7513)
11. Penicillin-Streptomycin (Gibco, 15140122)
12. Dissociation reagent e.g Trypsin/EDTA or TrypLE (e.g Gibco, 12605-010)
13. Biovision LDH-cytotoxicity assay kit (Biovision, K311-400)
14. PBS (Difco, BR0014)

5.3 Reagent Preparation

Cell culture medium:

The complete medium for LLC-PK1 should be made fresh every week and stored at 4°C. If it is not used within a week remaining media should be discarded. The complete cell culture

Document Type	Document ID	Version	Status	Page
SOP	EUNCL-GTA-001	1.0		4/15

media is prepared by adding 2 mM L-Glutamine, 3% FBS and 100 U/mL Penicillin-Streptomycin to Medium 199.

Positive Controls:

Prepare all positive controls fresh for each round of assay, same control can be used for all reading point (0, 4, 24 and 48 hr)

1. 0.1% Triton-X-100:

Prepare a 20X stock (2%) of Triton-X-100 by adding 2 mL of Triton-X-100 to 8 mL of Medium 199 Cell Culture Media (with 3% FBS). Sterilize by filtering through a 0.2 µm filter.

2. Digitonin stock solution is made by solubilizing digitonin in DMSO to a final concentration at 20 mg/mL. Mix until a clear and homogeneous solution is obtained. The stock solution can be aliquoted and frozen at -20°C. Prepare a 2X digitonin solution for internal plate control by diluting digitonin stock (20 mg/mL) in Medium 199 Cell Culture Media to a final concentration of 60 µg/mL.

MTT assay:

1. MTT solution:

Prepare 5 mg/mL MTT in PBS. Sterilize by filtering using a 0.2 µm filter. The solution can be stored for up to one month at 4°C in the dark, or freeze at -20 °C.

2. Glycine Buffer:

Prepare 0.1 M glycine (MW 75.07) with 0.1 M NaCl (MW 58.44) in MQ water, pH 10.5.

Sterilize by filtering using a 0.2 µm filter. The solution can be stored at room temperature for up to 4 weeks.

LDH assay:

1. Reconstitute catalyst in 1 mL dH₂O for 10 min with occasional vortexing. The solution is stable for 2 weeks at 4°C.

2. Reaction mixture (for one 96-well plate): Add 250 µL of reconstituted catalyst solution to 11.25 mL of dye solution. Once thawed, the kit components are stable for 2 weeks stored at 4°C. Reconstituted catalyst solution should be added to the dye solution immediately before use.

Document Type	Document ID	Version	Status	Page
SOP	EUNCL-GTA-001	1.0		5/15

6 Procedure

6.1 Flow chart

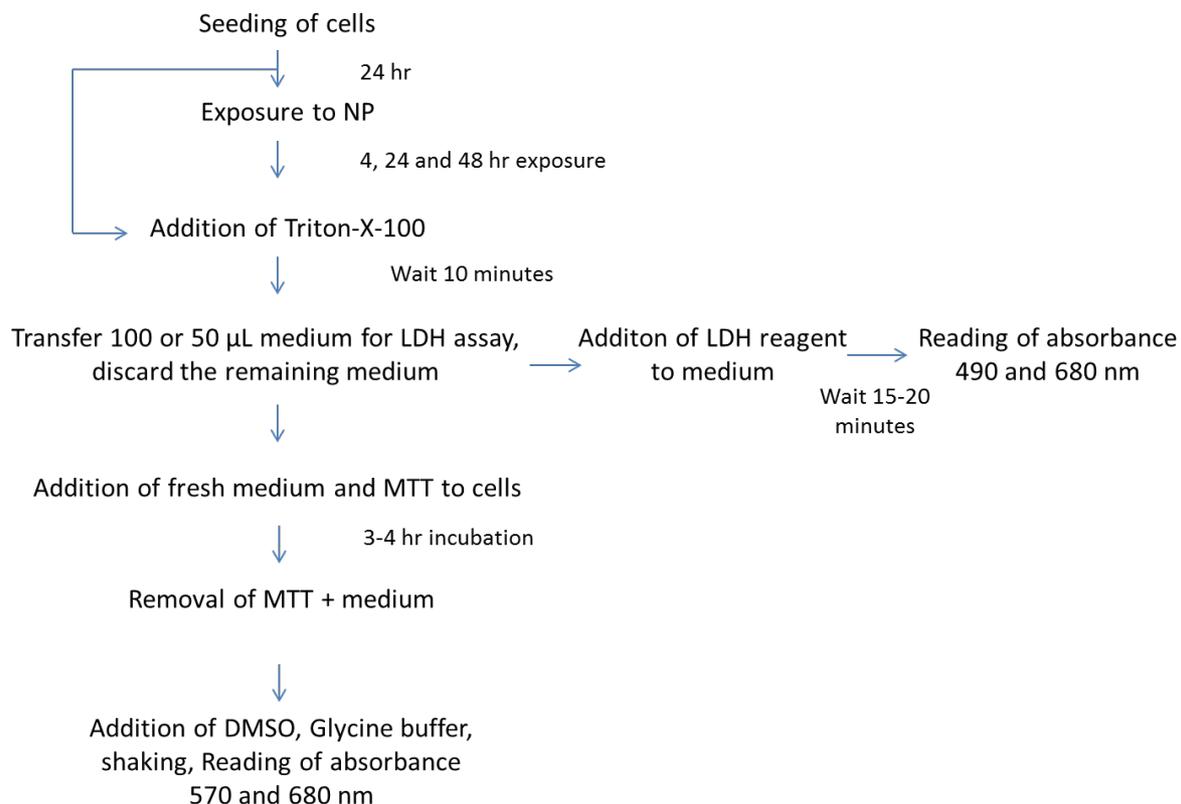


Figure 1: Brief outline of the workflow.

6.2 Cell handling

- The LLC-PK1 cell line used by EUNCL is obtained from LGC Standards, see Annex for detailed information about thawing and propagation of a set of stock ampoules.
- These stock ampoules serve as starting point for all experiments.
- After thawing of stock ampoules, cells are subcultured for 3 passages or more until enough amount of cells are achieved (see Subcultivation).
- On the day of experiment, perform cell seeding as described in 6.4, continue with addition of samples the following day as described in 6.5.

Subcultivation

Document Type	Document ID	Version	Status	Page
SOP	EUNCL-GTA-001	1.0		6/15

LLC-PK1 cells are kept in a sub confluent state by routinely passaging twice or three times a week to seeding densities between $1.2 \times 10^4 - 3.2 \times 10^4$ cells /cm².

Given volumes are for 75 cm² flask – proportionally reduce or increase amount of dissociation medium for culture vessel of other size.

1. Remove and discard culture medium.
2. Wash the cell layer twice by gently rinsing it with 10-15 mL preheated (37°C) Dulbecco's phosphate-buffered saline without calcium and magnesium.
3. Add 2.0-3.0 mL dissociation reagent (*e.g* Trypsin/EDTA or TrypLE®), incubate at 37°C for 10 minutes, and gently knock culture flasks to detach most of the cells.
4. Resuspend cells in medium containing FBS to stop trypsination.
5. Transfer and dilute in new culture vessels.
6. Incubate the culture at 37°C in a humidified atmosphere with 5% CO₂ in a suitable incubator.

6.3 Cell seeding

Cell preparation (or as recommended by supplier, see also 6.3.)

1. Harvest cells from prepared flasks, the cells should be cultivated for minimum 3 passages before use for experiment. **Note:** Limit to 20 passages from vial from cell bank at LGC Standards (Figure 3).
2. Count cell number using a coulter counter or hemocytometer.
3. Dilute cells to a density of 2.5×10^5 cells/mL in Medium 199 (3% FBS) cell culture media.
4. Plate 100 µL cells/well as per plate format (Annex) for four 96-well plates (time zero, 4, 24, and 48 hr sample exposure). See plate design.
5. Incubate plates for 24 hr at 5% CO₂, 37°C and 95% humidity. Cells are grown to approximately 80% confluence (Figure 2).

Document Type	Document ID	Version	Status	Page
SOP	EUNCL-GTA-001	1.0		7/15

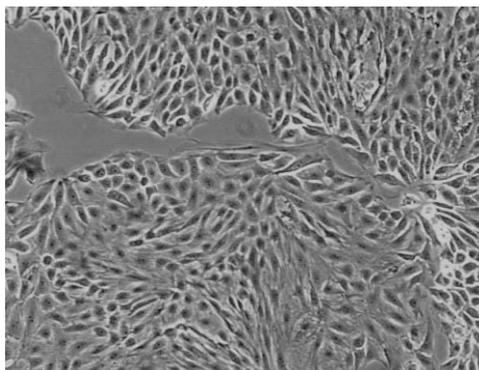


Figure 2. LLC-PK1 Cell Culture. Image was taken with a phase contrast microscope at 225X magnification. LLC-PK1 cells are approximately 80% confluent at this stage.

6.4 Assay procedure

The cells are prepared in 96-well plates as described in section 6.4. See also plate design in Annex. The format indicates no cells in rows A and H as they serve as particle blanks to be subtracted from cell treatment wells. Each plate accommodates two samples (Rows A–D and E–H). Each nanoparticle is tested at nine dilutions. Column 11 receives the Triton X-100 at the end of the relevant time point and column 12 receives the positive control Digitonin.

Time Zero Plate (MTT Assay)

1. Remove time zero plate from the incubator and add 100 μ L fresh culture media to all wells. Then add 10 μ L of 20X Triton-X-100 to the positive control wells in column 11 (see plate format in Annex) for a final concentration of 0.1% Triton-X-100 (see Section 5.3). Let the plate set for 10 minutes at room temperature.
2. Remove 100 μ L of media from each well and transfer it to another plate (Greiner, 655163), maintaining plate format. Transfer 50 μ L if half area plates are used for LDH assay (Costar, 3695). Use this plate immediately for the LDH assay (see Section below).
3. Remove remaining media from original plate and discard.
4. Add 200 μ L fresh media to all wells.
5. Add 50 μ L MTT (see Section 5.3) to all wells.
6. Cover with aluminum foil and incubate at 37°C for 3-4 hrs.
7. Aspirate and discard media.
8. Add 200 μ L DMSO to all wells to solubilize the MTT formazan crystals.

Document Type	Document ID	Version	Status	Page
SOP	EUNCL-GTA-001	1.0		8/15

9. Add 25 μL glycine buffer (see Section 5.3) to all wells. Cover with aluminum foil and place on shaker to mix for 10 minutes in room temperature.
10. Read absorbance at 570 nm on plate reader using a reference wavelength of 680 nm.

Test Samples and Positive Control Addition

All samples are run in triplicates with 9 dilutions each (see Plate Map).

1. The highest concentration of nanoparticle tested should be at the limit of solubility or determined by the potency of the test material.
2. Dilute the test compound in media, making a total of nine 1:4 dilutions at 2X of the desired final concentration. Different dilution series (i.e. 1:2, 1:10) can be done depending on test material potency and availability.
3. Add 100 μL of each sample dilution and positive control to 4, 24 and 48 hr exposure plates as per the plate format (Annex), and place in 37°C incubator with 5% CO_2 and 95% humidity for indicated time. Note that Triton X-100 control is added later at the end of the exposure time, so that these wells receive only 100 μL media at this point (See step 1 in MTT assay). Alternatively, sample and positive control can be made at desired final concentration. Media is aspirated from the wells on the test plates, and sample and positive control are added at 200 μL per well as per the plate format (Annex).

Test Plates, 4, 24 and 48 hr exposures (MTT Assay)

1. At the end of each exposure time point, remove plate from incubator and add 10 μL of 20X Triton-X-100 to positive control wells (see plate format in Annex) for a final concentration of 0.1% Triton-X-100 (see Section 5.3). Let the plate set for 10 minutes at room temperature.
2. Remove 100 μL of media from each well and transfer it to another plate (Greiner, 655163), maintaining plate format. Transfer 50 μL if half area plates are used for LDH assay (Costar, 3695). Use this plate immediately for the LDH assay (see Section below).
3. Remove remaining media from original plate and discard.
4. Add 200 μL fresh media to all wells.
5. Add 50 μL MTT to all wells.
6. Cover with aluminum foil and incubate for 37°C for 3-4 hr.
7. Aspirate and discard media.
8. Add 200 μL of DMSO to each well.

Document Type	Document ID	Version	Status	Page
SOP	EUNCL-GTA-001	1.0		9/15

9. Add 25 μL of glycine buffer to each well. Cover with aluminum foil and place on shaker to mix for 10 minutes in room temperature.
10. Read absorbance at 570 nm on plate reader using a reference wavelength of 680 nm.

Test plates, 0, 4, 24 and 48 hr exposures (LDH Assay)

(Adapted from Biovision LDH Cytotoxicity Assay Kit, K311-400)

1. Add 100 μL of the Reaction Mixture (see Section 5.3) to each well of transfer plate. Alternatively add 50 μL of the Reaction Mixture if half area plates are used. Shake plate on an orbital shaker briefly to mix samples.
2. Incubate at room temperature for up to 20 minutes in the dark.
3. Read the plate on a plate reader at 490 nm using a reference wavelength of 680 nm.

6.5 Calculations

All samples, positive, negative, and media controls are run in triplicate (e.g., rows B-D or E-G). Each well will be subtracted from its respective cell-free blank (e.g., B2-A2 or G3-H3) in the following calculations. The average of these three values should be used in the equations below for the positive and negative controls (e.g., $[(B10-A10) + (C10-A10) + (D10-A10)]/3$ = mean media control absorbance for sample 1, or $[(B11-A11) + (C11-A11) + (D11-A11)]/3$ = mean Triton-X-100 positive control absorbance for sample 1. Sample 2 uses the blank row H for subtractions.).

1. MTT Assay

$$\% \text{ Cell Viability} = \frac{\text{sample absorbance} - \text{cell free sample blank}}{\text{mean media control absorbance}} \times 100$$

2. LDH Assay

$$\% \text{ Total LDH Leakage} = \frac{(\text{sample absorbance} - \text{cell free sample blank}) - \text{mean media control absorbance}}{\text{mean TritonX positive control absorbance} - \text{mean media control absorbance}} \times 100$$

3. Mean, SD and %CV should also be calculated for each positive control, negative control and unknown sample.

7 Quality Control, Quality Assurance, Acceptance Criteria

Acceptance criteria

1. A set of assay wells exposed to a dilution series (9 dilutions, 3 parallel wells per concentration) of the positive control digitonin for 24 hours is included in each assay batch, starting at 140 $\mu\text{g}/\text{ml}$. The EC50 value of the digitonin positive control

Document Type	Document ID	Version	Status	Page
SOP	EUNCL-GTA-001	1.0		10/15

is used for monitoring of assay performance. Plot values for each assay batch.

Assays batches in which the EC50 value of the digitonin positive control are outside of 3 standard deviations should be discarded.

2. The viability in wells with the plate internal digitonin control should be less than 50 %.
3. The replicate coefficient of variations of the positive controls and of the samples should be within 50%.
4. The assay is acceptable if criteria 1 and 3 are met. Otherwise, the assay should be repeated until acceptance criteria are met.
5. If the acceptance criteria are met, determine the highest concentration of the nanoparticulate material that does not interfere with the assay system indicated in rows A and H.
6. The concentration–response curves for the 48 hr MTT and LDH data should be classified as having complete (two observed asymptotes) or incomplete (second asymptote not obtained) curves, single point activity (activity at the highest concentration only), or no activity. For all complete 48 hr concentration–response curves, a nonlinear fit of the sigmoidal Hill equation should be performed, and an estimate of potency (EC50 - Calculated using Graphpad Prism), efficacy (Emax), minimum response (E0), and Hill slope (γ) from the Hill equation (below) fit should be reported. Any excluded points (excluded by outlier analysis) should also be reported.

$$E = E_0 + [(E_{max} - E_0)C^\gamma / EC_{50} \cdot C^\gamma]$$

8 Health and Safety Warnings, Cautions and Waste Treatment

Please refer to available H.S.E information for any nano formulations evaluated in the assays. Note that some of the listed reagents are hazardous and must be handled with precaution. Please refer to safety data sheets for each reagent, wear protective equipment, and dispose waste according to local regulations.

9 Abbreviations

CV	coefficient of variation
DMSO	dimethyl sulfoxide
FBS	fetal bovine serum

Document Type	Document ID	Version	Status	Page
SOP	EUNCL-GTA-001	1.0		11/15

INT	2-(p-iodophenyl)-3-(p-nitrophenyl)-5-phenyltetrazolium chloride
LDH	lactate dehydrogenase
LLC-PK1	renal epithelial cell line, porcine kidney
MTT	3-(4,5-dimethylthiazol-2-yl)-2,5-diphenyltetrazolium bromide
MW	molecular weight
NaCl	Sodium Chloride
PBS	phosphate buffered saline
SD	standard deviation

10 References

1. ISO 10993-5, Biological evaluation of medical devices: Part 5, Tests for *in vitro* cytotoxicity.
2. F1903 – 98, Standard Practice for Testing for Biological Responses to Particles in vitro.
3. Alley, et al. (1988) Cancer Res. 48:589-601.
4. Decker, T. & Lohmann-Matthes, M.L. (1988) J. Immunol Methods 15:61-69.
5. Korzeniewski, C. & Callewaert, D.M. (1983) J. Immunol Methods 64:313-320.
6. Freshney, R. I. (2010). Culture of animal cells: a manual of basic technique and specialized applications. (pp. 87-88, 193) Hoboken, N.J., Wiley-Blackwell
7. NCL Method GTA-1, Version 1.2, November 2015
LGC Standards

Document Type	Document ID	Version	Status	Page
SOP	EUNCL-GTA-001	1.0		12/15

11 Appendix

11.1 Cell handling and storage

11.1.1 Cell origin and provenance

LLC-PK1 porcine proximal tubule cells are used as a functional model in the kidney cytotoxicity assay and must be well characterized and validated. Validated cell lines are obtained from LGC Standards. Upon arrival the LLC-PK1 cells should be propagated and cryopreserved at a low passage number. In order to minimize variations between EU-NCL labs due to cell cultivation, cell lines used in the EU-NCL-GTA01 assay should not be propagated above 20 passages from original vials from LGC Standards (See figure 3) [6, 7].

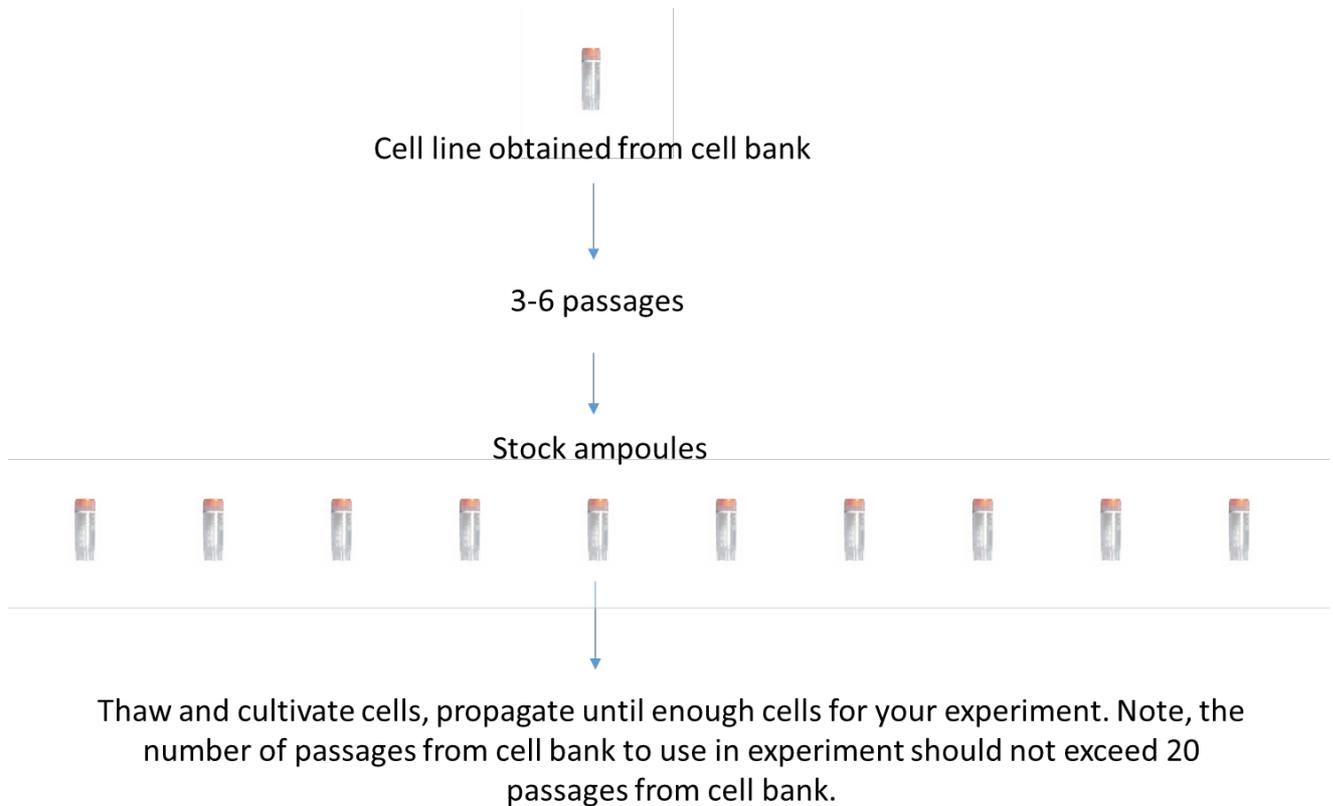


Figure 3: Propagation of stock ampoules from LGC Standards.

11.1.2 Thawing Procedure

Thawing of frozen ampoule was done according to instructions from cell bank [8].

1. Thaw the vial by gentle agitation in a 37°C water bath. To reduce the possibility of contamination, keep the O-ring and cap out of the water. Thawing should be rapid, approximately 1-2 minutes.
2. Remove the vial from the water bath as soon as the content is thawed, and decontaminate by spraying with 70% ethanol. Place the vial into biosafety cabinet and work under strict aseptic conditions.

Document Type	Document ID	Version	Status	Page
SOP	EUNCL-GTA-001	1.0		13/15

3. Transfer the vial content to a sterile 15 mL conical centrifuge tube containing 9.0 mL preheated complete culture medium, and spin at 140 x G for 5 minutes. Discard supernatant.
4. Resuspend the cell pellet gently in 2-3 mL of the complete cell medium (this small volume makes it easier to achieve a homogeneous suspension). Gently dilute the cell suspension to the recommended final volume in culture vessel.
5. Incubate the culture at 37°C in a humidified atmosphere with 5% CO₂ in a suitable incubator.

11.1.3 Propagation of stock ampoules

Stock ampoules were propagated by thawing vial from cell bank according to thawing procedure (11.2.2). For LLC-PK1 the vial from cell bank was thawed, old media containing freeze agent was removed by diluting in fresh media before spinning down the cells. Cell pellet was resuspended in fresh media and transferred to a T25 culture vessel. The cell line became 70-80% confluent after two days, and was passaged twice before freezing of stock ampoules.

P1: Thaw to 10 mL in T25 (2 days)

P2: Split and seed to 2.6×10^4 cells/cm² to T75 (1-2 days)

P3: Split and seed to 1.2×10^4 cells/cm² (3 days), freeze stock ampoules when cells become 70-80% confluent.

Freezing Procedure

Always start by preparing all reagents, vials and equipment needed for freezing cells. After the cells are out of the incubator, minimal time should be used for such preparation steps.

1. Harvest cells according to the description for subculturing. After dissociation of cells, dilute them in fresh culture medium.
2. Measure cell density and viability by taking out an aliquot of the cell suspension. Calculate the necessary volume of freezing media (See Freezing Media underneath).
3. Transfer cell suspension to centrifuge tubes, and spin down cells at 140 x G for 5-7 minutes. Avoid very dense cell suspensions as these might be difficult to spin down.
4. Remove all medium.
5. Gently resuspend cells to wanted concentration in fresh freezing medium. Freeze LLC-PK1 cells at $1 \times 10^6 - 2 \times 10^6$ cells/mL in cryogenic vials, aliquot 1 mL in each vial.
6. Transfer cryovials to freezing containers (CoolCell®), and place the container in -80°C freezer, leave for at least four hours before transferring to storage in liquid nitrogen.

Freezing Media

1. To prepare LLC-PK1 freezing media use complete supplemented medium and add sterile DMSO (Dimethyl sulfoxide Hybri-Max™ (Sigma, D2650 or equivalent) to a final volume of 5% (v/v).

Document Type	Document ID	Version	Status	Page
SOP	EUNCL-GTA-001	1.0		14/15

11.1.4 Plate map with positioning of samples and controls in assay plates

	1	2	3	4	5	6	7	8	9	10	11	12
A	Media TS1, D9	Media TS1, D8	Media TS1, D7	Media TS1, D6	Media TS1, D5	Media TS1, D4	Media TS1, D3	Media TS1, D2	Media TS1, D1	Media	Media Triton-X 0.1%	Media DIGI 30 µg/mL
B	Cells TS1, D9	Cells TS1, D8	Cells TS1, D7	Cells TS1, D6	Cells TS1, D5	Cells TS1, D4	Cells TS1, D3	Cells TS1, D2	Cells TS1, D1	Cells Media	Cells Triton-X 0.1%	Cells DIGI 30 µg/mL
C	Cells TS1, D9	Cells TS1, D8	Cells TS1, D7	Cells TS1, D6	Cells TS1, D5	Cells TS1, D4	Cells TS1, D3	Cells TS1, D2	Cells TS1, D1	Cells Media	Cells Triton-X 0.1%	Cells DIGI 30 µg/mL
D	Cells TS1, D9	Cells TS1, D8	Cells TS1, D7	Cells TS1, D6	Cells TS1, D5	Cells TS1, D4	Cells TS1, D3	Cells TS1, D2	Cells TS1, D1	Cells Media	Cells Triton-X 0.1%	Cells DIGI 30 µg/mL
E	Cells TS2, D9	Cells TS2, D8	Cells TS2, D7	Cells TS2, D6	Cells TS2, D5	Cells TS2, D4	Cells TS2, D3	Cells TS2, D2	Cells TS2, D1	Cells Media	Cells Triton-X 0.1%	Cells DIGI 30 µg/mL
F	Cells TS2, D9	Cells TS2, D8	Cells TS2, D7	Cells TS2, D6	Cells TS2, D5	Cells TS2, D4	Cells TS2, D3	Cells TS2, D2	Cells TS2, D1	Cells Media	Cells Triton-X 0.1%	Cells DIGI 30 µg/mL
G	Cells TS2, D9	Cells TS2, D8	Cells TS2, D7	Cells TS2, D6	Cells TS2, D5	Cells TS2, D4	Cells TS2, D3	Cells TS2, D2	Cells TS2, D1	Cells Media	Cells Triton-X 0.1%	Cells DIGI 30 µg/mL
H	Media TS2, D9	Media TS2, D8	Media TS2, D7	Media TS2, D6	Media TS2, D5	Media TS2, D4	Media TS2, D3	Media TS2, D2	Media TS2, D1	Media	Media Triton 0.1%	Media DIGI 30 µg/mL

Abbreviations:

TSX: Test sample number X

DX: Dilution number X

DIGI: Digitonin plate internal control sample

Document Type	Document ID	Version	Status	Page
SOP	EUNCL-GTA-001	1.0		15/15